



## Instructions for Installation of Trek Model 555P Series Probes in Vacuum Applications

The vacuum connector used must be of the high-voltage type due to the potential on the conductors of the cables reaching up to the value of the measured potential. In the case of using a 555P series probe connected to a Trek Model 344 or 347 Electrostatic Voltmeter, a potential up to  $\pm 3500$  volts can exist between all conductors, taken as a group, and EARTH GROUND. However, the maximum voltage between any conductor within the cable, and any other conductor within the cable, is limited to less than  $\pm 100$  volts.

The 555P series probe may be applied and operated under vacuum conditions up to at least  $10^{-6}$  Torrs. These vacuum applications are achieved by cutting the probe cable at the appropriate position which allows the proper cable length inside the vacuum chamber.

The procedure is as follows:

- A) Cut the cable at the appropriate position (which allows the proper cable length inside the vacuum chamber).
- B) Separate, dress, and solder the various cable connections for both ends of the cable using the following precautions:
  - 1. The shields for the WHITE, BLACK, and RED wires are at a common potential and therefore may be connected together as shown in page 2 Diagram as contact "B".

Electrical tape or heat-shrink tubing may be used to ensure that electrical separation is achieved and held between the connections.

- B) 2. If the shells of the high-voltage connector and its mating connector are of a conductive (metallic) material and these conducting shells are connected to EARTH GROUND due to their contact to the vacuum (metallic) chamber walls, care must be taken to ensure that all conductors of the probe cable have sufficient clearance to these shells to prevent arc over between the cable and the shells.

The sufficient clearance must support a clearance of up to  $\pm 3500$  volts.

**NOTE:** Pin designations A, B, C, and D, are used for reference purposes only and do not necessarily describe the actual pin designations on the particular connector being used.

Copyright © 2005 TREK, INC.


**CONTROL WITHOUT COMPROMISE**

TREK, INC. 190 Walnut Street • Lockport, NY 14094 • 800-FOR TREK  
716-438-7555 • 716-201-1804 (fax) • www.trekinc.com • sales@trekinc.com



Page 1 of 2  
0522/JNC  
Rev. 0

Trek Model 555P Series Probes in Vacuum Applications Diagram

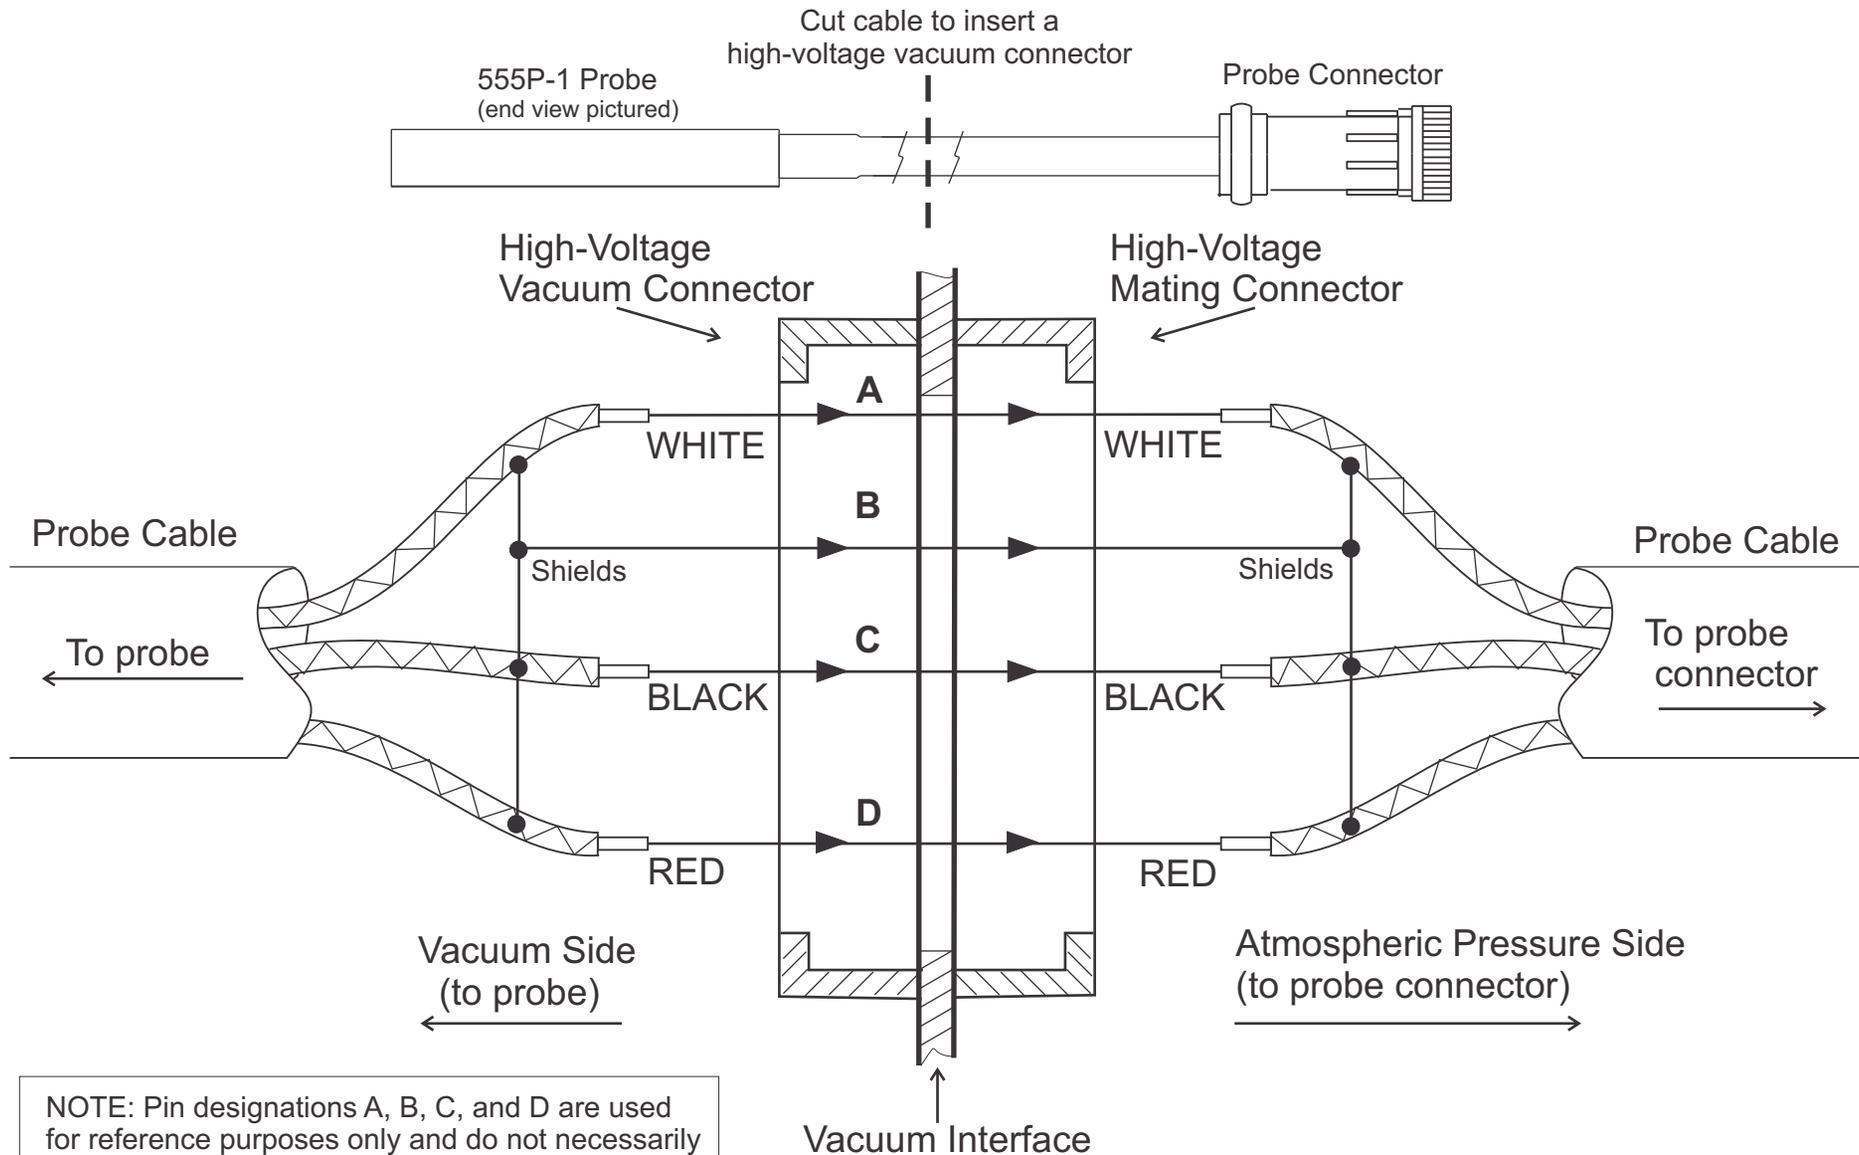

NOTE: Pin designations A, B, C, and D are used for reference purposes only and do not necessarily describe the actual pin designations on the particular connector being used.